

Distal Femur Outcomes in High Risk Patients*

Stainless Steel Plate

vs.

Carbon Fiber PEEK Plate




PATIENT OUTCOME
75% BONE UNION

PATIENT OUTCOME
100% BONE UNION




COMPLICATIONS
8% HARDWARE FAILURES

COMPLICATIONS
0% HARDWARE FAILURES



PATIENT RISK FACTORS
13% DIABETES
0% PVD+
54 AVG. AGE


PATIENT RISK FACTORS
57% DIABETES
43% PVD+
68 AVG. AGE

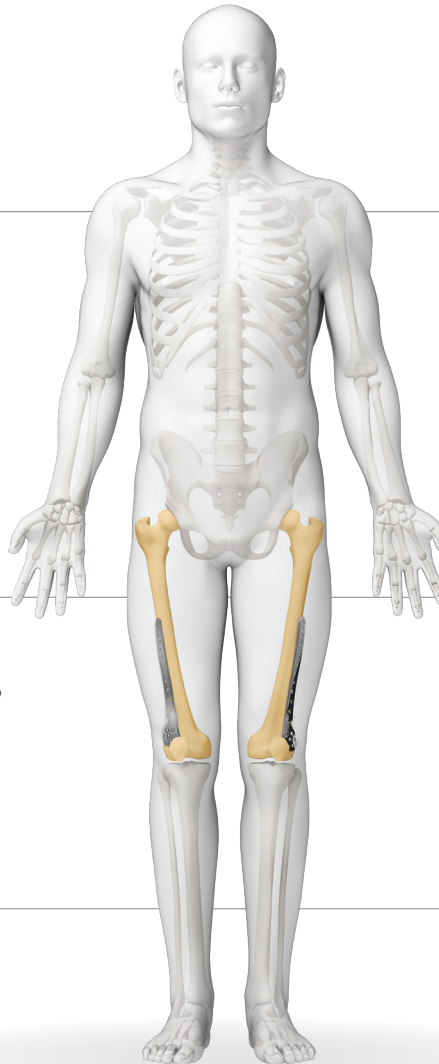

CLINICAL EXPERIENCE

17 Publications covering 398 Cases*

ANATOMIC LOCATIONS AND NUMBER OF CASES

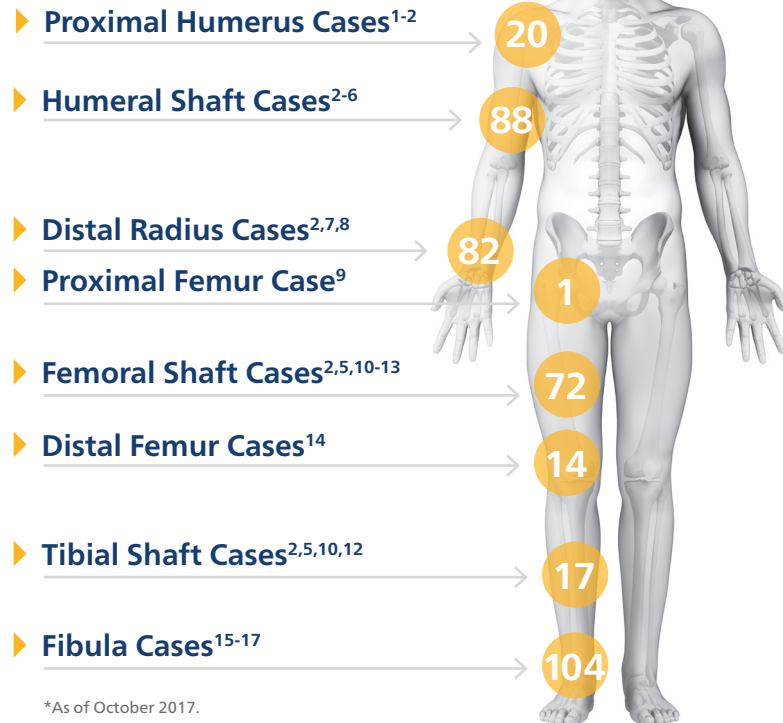

*As of October 2017.

REFERENCES

- Hak, DJ et al. Seeing is believing: treatment of proximal humerus fractures using a novel radiolucent implant and its effect on reduction accuracy, healing rate and functional outcome. Paper #482. Presented at EFORT 2014 Annual Meeting.
- Rosenthal H. Invisible Stabilization of Impending and Pathological Fractures A Preliminary Report on Carbon Fiber Technology. Presented at: MSTs Annual Meeting 2013.
- Collis P, Clegg T, Seligson D. The invisible nail: A technique report of treatment of a pathological humerus fracture with a radiolucent intramedullary nail. *Injury*. 2011 Apr; 42(4):424-6.
- Kojic N, et al. Carbon-Fibre-Reinforced PEEK radiolucent intramedullary nail for humeral shaft fracture fixation: technical features and a pilot clinical study. *Injury*. 2017 Nov;48 Suppl 5:S8-S11.
- Piccioli A, Piana R, Lisanti M, et al. Carbon-fiber reinforced intramedullary nailing in musculoskeletal tumor surgery: a national multicentric experience of the Italian Orthopaedic Society (SIOT) Bone Metastasis Study Group. *Injury*. 48. S55-S59.
- Caforio M. The Carbon Fiber Intramedullary Nail in Pathological Humeral Shaft Fractures: Two Case Reports. *J J Ortho Rheum*. 2015, 1(2): 008.
- DiMaggio B, et al. PEEK radiolucent plate for distal radius fractures: multicentre clinical results at 12 months follow up. *Injury*. 2017 Oct;48 Suppl 3:S34-S38.
- Perugia D, et al. Comparison between Carbon-Peek volar locking plates and titanium volar locking plates in the treatment of distal radius fractures. *Injury*. 2017 Oct;48 Suppl 3:S24-S29.
- Zoccali C, et al. The CarboFix™ "Piccolo Proximal femur nail": a new perspective for treating proximal femur lesion. A technique report. *J Orthop*. 2016 Jul;13(4):343-6.
- Allison DC, Menendez LR. Carbon fiber fixation in oncologic bone surgery. Presented at MTS Meeting 2013.
- Prince DE, Paley D, Harris M. Case Report: Use Of Carbon Fiber Intramedullary Nail And External Fixation Assistance For Treatment Of Osteoid Osteoma. Presented at MTS Annual Meeting 2013.
- Zimel MN, Hwang S, Riedel ER, Healy JH. Carbon fiber intramedullary nails reduce artifact in postoperative advanced imaging. *Skeletal Radiol*. 2015 Sep;44(9):1317-25.
- Ziran BH, Mansour J, Jahangir AA, Min W. Efficacy of Carbon Fiber-Reinforced PEEK Femoral Nails: Preliminary Results. Poster #68. Presented at OTA 2017.
- Lee AK, Mitchell PM, Ziran BH, Jahangir AA. Early Comparative Outcomes of Continuous Carbon Fiber-Reinforced Polymer Plate in Fixation of Distal Femur Fractures. Paper #155. Presented at OTA 2017.
- Caforio M, et al. Preliminary experience with Piccolo Composite™, a radiolucent distal fibula plate, in ankle fractures. *Injury*. 2014 Dec;45 Suppl 6:S36-S38.
- Guzzini M, Lanzetti RM, Lupariello D, et al. Comparison between carbon-peek plate and conventional stainless steel plate in ankle fractures. A prospective study of two years follow up. *Injury*. 2017 Jun;48(6): 1249-1252.
- Pinter ZW, Smith KS, Hudson PW, et al. A Retrospective Case Series of Carbon Fiber Plate Fixation of Ankle Fractures. *Foot Ankle Spec*. 2017 Jul 1 :1938640017718343.

For further information call us toll free at 866-INVIBIO or +44 (0)1253 898000 or please visit our website at:

▶ **Invibio.com**

Victrex plc and/or its group companies ("Victrex plc") believes that the information contained in this document is an accurate description of the typical characteristics and/or uses of the product or products, but it is the customer's responsibility to thoroughly test the product in each specific application to determine its performance, efficacy, and safety for each end-use product, device or other application. Suggestions of uses should not be taken as inducements to infringe any particular patent. The information and data contained herein are based on information we believe reliable. Mention of a product in this document is not a guarantee of availability.

Victrex plc reserves the right to modify products, specifications and/or packaging as part of a continuous program of product development. Victrex plc makes no warranties, express or implied, including, without limitation, a warranty of fitness for a particular purpose or of intellectual property non-infringement, including, but not limited to patent non-infringement, which are expressly disclaimed, whether express or implied, in fact or by law.

Further, Victrex plc makes no warranty to your customers or agents, and has not authorized anyone to make any representation or warranty other than as provided above. Victrex plc shall in no event be liable for any general, indirect, special, consequential, punitive, incidental or similar damages, including without limitation, damages for harm to business, lost profits or lost savings, even if Victrex has been advised of the possibility of such damages regardless of the form of action.

Supporting information is available on request for all claims referenced in this document.

Copyright © 2018 Invibio Ltd. INVIBIO™, PEEK-OPTIMA™, INVIBIO BIOMATERIAL SOLUTIONS™ are trademarks of Victrex plc or its group companies. All rights reserved.